



# **Influence of soft tissue in the assessment of the primary fixation of acetabular cup implants using impact analyses**

Romain Bosc, Antoine Tijou, Giuseppe Rosi, Vu-Hieu Nguyen, Jean-Paul Meningaud, Philippe Hernigou, Charles Henri Flouzat Lachaniette, Guillaume Haiat

## **► To cite this version:**

Romain Bosc, Antoine Tijou, Giuseppe Rosi, Vu-Hieu Nguyen, Jean-Paul Meningaud, et al.. Influence of soft tissue in the assessment of the primary fixation of acetabular cup implants using impact analyses. Clinical Biomechanics, 2018, 55, pp.7-13. 10.1016/j.clinbiomech.2018.03.013 . hal-01786001

**HAL Id: hal-01786001**

**<https://hal.science/hal-01786001>**

Submitted on 4 May 2018

**HAL** is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.

**Influence of soft tissue in the assessment of the primary fixation of acetabular cup  
implants using impact analyses**

---

Romain Bosc<sup>a,b</sup>, Antoine Tijou<sup>c</sup>, Giuseppe Rosi<sup>c</sup>, Vu-Hieu Nguyen<sup>c</sup>, Jean-Paul Meningaud<sup>b</sup>,  
Philippe Hernigou<sup>d</sup>, Charles-Henri Flouzat-Lachaniette<sup>d</sup>, Guillaume Haiat<sup>c</sup>

<sup>a</sup>INSERM U955, IMRB Université Paris-Est, 51 avenue du Maréchal de Lattre de Tassigny, 94000  
Créteil, France

<sup>b</sup>Hopital Henri Mondor. Plastic, Reconstructive, Aesthetic and Maxillofacial Surgery Department.  
50, avenue du Maréchal de Lattre de Tassigny 94000, Créteil, France

<sup>c</sup>Laboratoire de Modélisation et de Simulation Multi-Echelle, UMR 8208, 61 Avenue du Général  
de Gaulle, Créteil 94010, France.

<sup>d</sup>Service de Chirurgie Orthopédique et Traumatologique, Hôpital Henri Mondor AP-HP, CHU  
Paris 12, Université Paris-Est, 51 avenue du Maréchal de Lattre de Tassigny, 94000 Créteil,  
France.

In preparation for Clinical Biomechanics

Corresponding author:

Romain Bosc

Henri Mondor Hospital, Assistance Publique des Hopitaux de Paris  
Plastic, Reconstructive, Aesthetic and Maxillofacial Surgery  
51, avenue du Maréchal de Lattre de Tassigny  
94000, Créteil, France

[Romainbosc@gmail.com](mailto:Romainbosc@gmail.com)

Abstract :247 words

Manuscript :3997 words

27 Contributions

28 Each author has materially participated in the research and the article preparation.

29 - The conception and design of the study: Guillaume Haiat and Antoine Tijou

30 - Acquisition and analysis of data: Romain Bosc and Antoine Tijou

31 - Interpretation of data: Romain Bosc, Charles-Henri Flouzat Lachaniette and Guillaume Haiat

32 - Draft: Romain Bosc, Antoine Tijou and Pr Hernigou

33 - Revising: Jean-Paul Meningaud, Philippe Hernigou and Guillaume Haiat

34 - Final Version : Antoine Tijou, Giuseppe Rosi and Vu-Hieu Nguyen.

35

36 All authors have approved the final article.

37

38 All authors disclose not any financial or personal relationships with other people or organizations  
39 that could inappropriately influence their work.

40

41

42

43

44

## Abstract

### *Background*

The acetabular cup implant primary stability is an important determinant for the long-term success of cementless hip surgery. However, it remains difficult to assess the implant fixation due to the complex nature of the bone-implant interface. A method based on the analysis of the impact produced by an instrumented hammer on the ancillary has been developed by our group (1). The aim of this study is to evaluate the influence of the soft tissue thickness on the acetabular cup implant primary fixation evaluation using impact analyses.

### *Methods*

To do so, different implants were inserted in three bovine bone samples. For each sample, different stability conditions were obtained by changing the cavity diameter. For each configuration, the acetabular cup implant was impacted 25 times with 10 and 30 mm of soft tissues positioned underneath the sample. The averaged indicator  $I_m$  was determined based on the amplitude of the signal for each configuration and each soft tissue thickness. The pull-out force was measured using a pull-out test.

### *Findings*

The results show that the resonance frequency of the system increases when the value of the soft tissue thickness decreases. Moreover, an ANOVA analysis shows that there was no significant effect of the value of soft tissue thickness on the values of the indicator  $I_m$  ( $F=9.45$ ;  $p\text{-value}=0.64$ ).

### *Interpretation*

This study shows that soft tissue thickness does not alter the prediction of the acetabular cup implant primary fixation obtained using the impact analysis approach, opening the path towards future clinical trials.

**Keywords:** Biomechanics; Acetabular cup implant; hip prosthesis; bone; impact; implant stability.

## Introduction

Press-fit surgical procedures are widely used in clinical practice to insert cementless acetabular cup (AC) implant into pelvic bone tissue (2,3). The aseptic loosening resulting from the partial or total absence of osseointegration remains one of the major causes of surgical failure (4–6) and depends on the primary stability of the AC implant. The AC implant primary fixation is an important determinant of the surgical success and it depends in turns on many factors such as the patient bone quality, the implant properties (e.g. surface treatment, implant geometry) and the surgical protocol. The choice of the implant size, the shape and diameter of the cavity reamed into bone tissue as well as the number and magnitude of the impacts used to insert the AC implant are important parameters determining the surgical outcome. The surgeons should find a compromise between a sufficient AC implant fixation in order to avoid micromotions at the bone implant interface (7), which may lead to fibrous tissue formation, and an excessive pre-stressed state of bone tissue (8) around the AC implant, which may lead to bone tissue necrosis. Moreover, while inserting the AC implant into bone tissue, the energy of the impacts should be sufficient high to eventually obtain a good primary stability but should not be too important to avoid acetabulum bone fracture (9). In case of insufficient initial stability during surgery, the surgeon may cement and/or screw the implant to help to osseointegration.

Despite the importance of the AC implant primary fixation, it remains difficult to be assessed quantitatively in the operating room. Various biomechanical tests such as pull-out tests (3,10–15) have been employed *in vitro* to evaluate the AC implant stability but such procedure cannot be used during the surgery. Vibrational techniques have been used to estimate the implant primary stability (16–20) but such an approach has not led so far to the development of a standardized method that can be employed intraoperatively. Classical medical imaging techniques such as magnetic resonance imaging or X-Ray microcomputed tomography are limited to provide quantitative information related to the stability of the AC implant because of diffraction phenomena around titanium. Moreover, such imaging techniques are still difficult to be used routinely during the surgery (21).

Orthopedic surgeons usually employ an empirical approach based on their experience and proprioception to estimate the AC implant primary stability, for instance by listening to the noise produced by the impact between the hammer and the ancillary (22) in order to adapt their strategy and to obtain an appropriate implant stability while avoiding per operative bone fractures (23).

A method has been developed by our group in order to obtain quantitative information on the AC insertion and fixation based on the analysis of the time variation of the force imposed to the ancillary supporting the AC implant during its impaction into bone tissue (24). This approach uses

an instrumented hammer in order to record the time dependence of the force during a given impact. An indicator, referred hereafter as impact momentum, has been defined and tested with reproducible mass fall (25). A correlation between the AC primary stability and the impact momentum was evidenced (26) and the approach was extended in order to account for the use of an instrumented hammer (1). All the aforementioned studies were realized with bovine bone specimens fixed in a clamp in order to work under reproducible conditions as far as practicable. The same approach was then validated in cadavers, in a situation closer to that of the operating room (27). Moreover, finite element models have been used in order to understand the dynamic biomechanical phenomena occurring during the impacts (8).

The radiofrequency (rf) signals corresponding to the variation of the force applied between the hammer and the ancillary as a function of time were qualitatively different when the experiments were carried out with a bone sample clamped on a rigid frame (1) and with cadavers (27), which shows the influence of the environment (such as for example the presence of soft tissues) on the measurements. Despite the aforementioned difference, the influence of the presence of soft tissues on the results of the method remains unexplored because it is difficult to determine quantitatively the thickness of soft tissues when working with cadavers. It is important to determine the influence of soft tissues on the measurements since it could jeopardize future measurements that could be carried out in the operating room to determine the AC implant stability when working with patients with varying body mass index for instance.

The aim of this paper is to examine the effects of soft tissue thickness (STT) on the impact momentum and estimate the influence of STT on the AC primary stability evaluation using impact analyses. To do so, three bone samples were considered *in vitro* with several drilling and AC sizes conditions and the value of STT was varied for all 48 different configurations considered.

## Methods

### 1. Acetabular cup implant, bone samples and soft tissues

Three bovine femurs were prepared similarly to what was done in the protocol described in Michel et al. (1). Briefly, each bone sample was embedded in a fast hardening resin (polymer SmoothCast 300, Smooth-On, Easton, PA, USA) for better handling and positioning, as shown in Fig. 1. All bone samples were made of trabecular bone in the region of the AC implant insertion.

Two slices of turkey breast were cut in order to obtain a thickness of 10 mm of soft tissues when one slice only was positioned underneath the sample and of 30 mm when both slices were employed. As schematized in Fig. 1, two beams located around the bone sample allow a translation along the vertical direction without friction (which was obtained through lubrication) of the bone sample during the impacts, similarly as in the clinical situation.

Two AC implants of diameter 52 and 54 mm (Pinnacle by Depuy, a Johnson & Johnson company, Warsaw, IN, USA) were employed. The AC implants were made of titanium alloy and coated with DUOFIX®, a combination of porous coating and highly amorphous hydroxyapatite. The AC cups were screwed to the dedicated ancillary and used similarly as in the operating room by an experienced surgeon.

### 2. Hammer impaction procedure

An impaction procedure corresponds to 25 successive impacts with the constraint that the maximum amplitude of the force should be comprised between 2500 and 4500N, which corresponds to a relatively weak impact compared to typical forces recorded during impacts employed to insert the AC implant (typically around 15 kN (28)). For each impact, the ancillary was held manually and impacted by the hammer ( $m = 1.3$  kg). A dynamic piezoelectric force sensor (208C05, PCB Piezotronics, Depew, New York, USA) with a measurement range up to 22 kN in compression was screwed in the center of the hammer impacting face. A data acquisition module (NI 9234, National Instruments, Austin, TX, USA) with a sampling frequency of 51.2 kHz and a resolution of 24 bits was used to record the time variation of the force applied between the hammer and the ancillary for each impact. The data were transferred to a computer and recorded using a LabVIEW interface (National Instruments, Austin, TX, USA) for a duration of 10 ms.

### 3. Signal processing

A dedicated signal processing technique was developed in order to extract information from the *rf* signal corresponding to the time variation of the force applied between the hammer and the ancillary. Similarly as in the *in vitro* study of Michel et al. (1), a quantitative indicator *I* referred to as impact momentum was determined for each impact following:

$$I = \frac{1}{A_0 \cdot (t_2 - t_1)} \int_{t_1}^{t_2} A(t) \cdot dt$$

where *A(t)* is the variation of the force applied between the hammer and the ancillary as a function of time,  $t_1=0.31$  ms and  $t_2=0.63$  ms.  $A_0$  was arbitrarily set equal to 1200 N in order to obtain values of the indicator *I* comprised in the interval [0;1]. The choice of the values  $t_1$ ,  $t_2$  and  $A_0$  will be discussed in section 4. Matlab (The Mathworks, Natick, MA, USA) was used to analyze the data.

#### 4. Tangential stability mechanical test

The AC implant fixation was assessed using a tangential stability mechanical test, similarly as in the previous studies of Michel et al. (1,26). The top end of the ancillary underwent a gradually increasing force (step of around 8 N.s<sup>-1</sup>) applied perpendicularly to its axis, with the bone sample rigidly clamped. The maximum value *F* of the force necessary to extract the AC implant from the bone sample was determined using a numerical dynamometer (DFX2- 050-NIST, AMETEK, Elancourt, FRANCE).

#### 5. Experimental protocol

Figure 2 summarizes the experimental protocol carried out by a trained surgeon, which aims at investigating different configurations with various values of AC implant stability and to compare the results obtained with 10 mm and 30 mm of STT.

A 49 mm diameter cavity was initially drilled in each bone sample using the reamer recommended by the implant manufacturer. A 52 mm diameter implant was inserted into bone tissue, leading to an interference diameter fit equal to three millimeters. The AC implant was inserted into bone tissue by several impactions until the surgeon considered that the implant could not be further inserted without significantly damaging the surrounding bone tissue. The hammer impaction procedure described in subsection II.2 and corresponding to 25 impacts with relatively low energy was then carried out with one slice of soft tissue positioned under the bone sample (STT=10 mm) and then with two slices of soft tissue (STT= 30 mm). For each impact, the value of the indicator *I* was computed as described in section 2.3. For each value of STT, the average value of the indicator *I* obtained for the 25 impacts was determined and noted  $I_m$ . Then, the tangential stability test



described in subsection 2.4 was carried out to determine the corresponding AC implant stability noted  $F$ .

The procedure described above including i) the implant insertion, ii) the impaction procedure (25 impacts) with the determination of the averaged values  $I_m$  of the indicator  $I$  for the two values of STT and iii) the tangential stability test was then repeated three times with the same 52 mm diameter implant, leading to a total number of four values for the pull-out force and of eight values for  $I_m$ .

The cavity was then enlarged from a diameter of 49 mm to a value of 51 mm using a dedicated reamer and the same procedure as the one described above was carried out with a 52 mm diameter implant to obtain an interference fit of 1 mm leading to another set of four values for the pull-out force and of eight values of  $I_m$ .

The same procedure was again reproduced without modifying the cavity using a 54 mm diameter AC implant. Eventually, a last round of experiments was realized using the same 54 mm diameter implant after having increased the size of the cavity up to a diameter of 53 mm using the dedicated burr.

The same protocol described above was carried out for the three bovine femoral bone samples, leading to a total number of 48 values of pull-out forces and 96 values of  $I_m$  which corresponds to three bone samples, three cavity diameters (49, 51 and 53 mm), two AC implant diameters and four measurements for each configurations (see Fig. 2). We verified that no fracture was present in the bone samples at all times.

## 6. Statistical analyses

The relationship between  $I_m$  and  $F$  was analyzed with linear regression analyses for each value of STT. An N-way analysis of variance and a multiple comparison test using the Tukey's Honestly Significant Difference method were performed to study the effect of the STT on the value of the averaged indicator  $I_m$ .

## Results

Figure 3 shows different averaged rf signals corresponding to the force applied between the hammer and the ancillary measured after the AC implant insertion (*i.e.* during the impaction procedure) for a given bone sample under various conditions. The black (respectively grey) lines correspond to a STT equal to 10 mm (respectively 30 mm). The solid lines shows the results obtained for an AC implant diameter equal to 52 mm and to a cavity diameter equal to 49 mm, which corresponds to an implant pull-out force equal to 31 N. The dashed (respectively dotted) lines shows the results obtained for an AC implant diameter equal to 52 mm (respectively 54 mm) and to a cavity diameter equal to 51 mm, which correspond to an implant pull out force equal to 63.4 N (respectively 72.8 N).

The results show that the rf signal exhibits i) a first maximum occurring just after the impact (around  $t=0.25$  ms), ii) a second maximum between 0.6 and 1 ms and iii) a third maximum between 3.0 and 5.5 ms. As shown in Fig. 3, the different rf signals around the first maxima ( $\sim 0.25$  ms) are qualitatively similar for all data obtained. However, the rf signals are significantly different around the second (0.6 - 1 ms) and the third maxima (3 - 5.5 ms). More specifically, the times of the second and third maxima are shown to increase when the AC implant stability increases, which is consistent with the results obtained in previous studies (1,25,26).

As shown in Fig 3, the time of the second maximum is slightly higher for configurations with STT equal to 30 mm compared to 10 mm. Similar results were obtained for most configurations (39 configurations out of 48). Figure 3 also shows that the time of the third maximum is always significantly higher for the results obtained with 30 mm of STT compared to the results obtained with 10 mm of STT. Similar results are obtained for almost all configurations (47 out of 48).

Figure 4 shows the results obtained when all data obtained from all bone samples and all configurations are pooled together. The circles (respectively the stars) show the data corresponding to a value of STT equal to 10 mm (respectively 30 mm). A significant correlation is obtained between the averaged values  $I_m$  of the indicator  $I$  and the tangential stability  $F$  for the configuration with 10 mm of STT ( $R^2=0.77$ ,  $p=2.6 \cdot 10^{-16}$ ). The same result was obtained for STT values equal to 30 mm ( $R^2 = 0.78$ ,  $p= 4.3 \cdot 10^{-17}$ ). Note that the two linear regression lines corresponding to the two values of STT are almost confounded.

The average and standard deviation values of the indicator  $I_m$  obtained for all samples and all configurations for a value of STT equal to 10 mm (respectively 30 mm) was equal to  $0.482 \pm 0.186$  (respectively  $0.465 \pm 0.186$ ). An ANOVA analysis shows that there was no significant effect of the value of STT on the values of the indicator  $I_m$  ( $F=9.45$ ;  $p$ -value=0.64). This result is confirmed by the multiple comparison tests ( $F=0.22$ ;  $p=0.64$ ).

Figure 5 shows the different values of the indicator  $I$  (black segments) and of the pull-out force (grey segments) for each values of implant and cavity diameters. The averaged and standard deviation values of  $I$  are shown as a function of the STT (10 and 30 mm). The results shown in Fig. 5 correspond to average values obtained for 4 sets of experiments (see Fig. 2) with different AC implant insertion conditions, which may explain the relatively important reproducibility obtained. As shown in the Fig. 5, the results are not significantly different when comparing the two values of STT for each configuration. Moreover, the highest values of pull-out force and of the indicator  $I$  are obtained when the interference fit is equal to 1 mm, which correspond to an AC implant (respectively cavity) diameter equal to 52 mm (respectively 51 mm) and to an AC implant (respectively cavity) diameter equal to 54 mm (respectively 53 mm).

## Discussion

The originality of the approach developed in this study is to provide in real time a way to estimate the AC implant primary fixation using an impact hammer in a non-invasive manner. Information provided by such impact hammer could be used in the future in a patient specific manner as a decision support system to determine whether the surgeons should modify the bone cavity, use screws or whether cementation is necessary. Moreover, the surgical protocol is not modified by the procedure.

In the literature, others techniques have been described to monitor the implants stability. Biomechanical techniques have been used to monitor dental implant primary stability (29,30) and bone integration (31) as well as the hip stem insertion endpoint (16) and primary stability (23,32). Vibrationnal technique have been tested to evaluate the AC implant primary stability (18). However, to the best of our knowledge, no accurate medical device can be used so far during surgery to assess the AC implant primary stability. Previous papers by our group have shown that the impact hammer could be employed with AC implant inserted in clamped bone samples (1) as well as in cadavers (27). The originality of the present study is to consider the effect of the STT on the indicator  $I$ . The results show that no significant effect of the STT on the indicator  $I$  has been obtained, which indicates that the measurements can be realized with any values of STT in the tested range (10-30 mm).

Although the correlation between the indicator  $I$  and the AC implant fixation has been shown not to depend on the STT, the rf signal itself depends on the STT, as shown in Fig. 3. In particular, the time of second maximum (between 0.6 and 1.0 ms in Fig. 3) of the rf signal is more often lower for 1 cm of STT compared to the results obtained with 3 cm of STT. The results are even more significant when considering the third maximum of the rf signal (between 3 and 5.5 ms in Fig. 3) because almost all configurations (except one) are concerned and because the time difference between the third maxima obtained with STT values equal to 10 and 30 mm is higher compared to the results obtained with the second maximum (see Fig. 3). The qualitative variation of the rf signals obtained with different STT may be explained by the fact that adding soft tissue to the tested system induces a decrease of its overall rigidity, thus resulting in a decrease of its resonance frequency. It has been shown experimentally (27), analytically (25), and numerically (8), that the frequency of the rf signal is determined by the rigidity of the system composed by the bone sample, the implant and the ancillary. Therefore, an increase of rigidity (corresponding to a decrease of STT) induces an increase of the resonance frequency and hence a decrease of the time of the different maxima of the rf signal, which is more important for higher order maxima. Despite this dependence of the rf signal

to soft tissue thickness, the indicator  $I$  is shown to weakly depend on the soft tissue thickness, which can be explained by the fact that the indicator is determined for relatively weak values of the time.

Different pull-out tests have been employed in the literature to assess the AC implant primary stability (33). We have chosen a tangential stability test because of its simplicity and because it has been already used in previous papers (5,34,35). In this study, the highest values of the pull-out force were obtained for an interference fit equal to 1 mm, which is consistent with previous studies (5) and with the recommendation of the implant manufacturer (8,36). A value of 1 mm for the interference fit is known to provide an adequate primary stability conditions of the AC implant (5,36). The effects of the interference fit on the AC insertion parameters have already been studied (8) and authors have concluded that a compromise has to be found between a sufficiently high value of the interference fit to ensure the AC stability and a sufficiently low value to avoid too important polar gaps and heterogeneous distribution of stresses within bone tissue (37,38).

Several parameters were chosen empirically in this study. First, the range of the maximum force (2500-4500 N) corresponding to the impacts used to determine the indicator, which is similar to what was done in (1), was chosen to obtain a compromise between a sufficiently low energy in order to avoid modifications of the implant insertion and/or of the bone-implant interface properties and a sufficiently high energy to obtain accurate measurement of the second and third maximum and to retrieve information on the bone-implant interface.

Second, the values of  $t_1 = 0.31$  ms and  $t_2 = 0.63$  ms were chosen approximately in the same range compared to previous studies (24) because the rf signals obtained herein are qualitatively similar to the ones obtained by Michel and al. (1). Note that the upper bound of the interval chosen in the present study (0.63 ms) is slightly lower compared to what has been done previously (1) so that the higher value of the time of the second maximum does not influence the results. However, the difference of the value of the upper bound of the interval does not significantly modify the results. Moreover, an optimization study was run to maximize the correlation coefficient between  $I$  and  $F$ . Changing the values of  $t_1$  between 0.28 and 0.35 ms or the value of  $t_2$  between 0.59 and 0.67 ms did not affect significantly the results (less than 3% difference for  $R^2$ , data not shown).

Third, the values of STT (10 and 30 mm) were selected because in our surgical experience, it could correspond approximately to the typical thickness of the soft tissues around the acetabulum.

337 This study has several limitations. First, the biomechanical properties of living human soft  
338 tissues may be different from the soft tissues used in our protocol. Turkey breast slices were chosen  
339 as a model of soft tissues because of their constant thickness and of their relative homogeneity in  
340 order to facilitate the interpretation of the data and the reproducibility of the results. It is therefore  
341 necessary to carry out future studies by an identical analysis on cadavers and then in real clinical  
342 situations.

343 Second, the biomechanical properties of human acetabular bone and of bovine femoral bone are also  
344 different, but of the same order of magnitude than bovine femoral bone (3,39). We considered bovine  
345 bone because of the large size of the epiphysis of the bovine femur which allows an easy and  
346 appropriate positioning of the AC implant (3,39).

347 Third, the value of the cavity diameter was not measured precisely for each impaction series. The  
348 cavities were realized manually, which also leads to imperfections in the shape of the cavity.  
349 Variations in the cavity diameter value may occur during the protocol run. However, such variations  
350 are also likely to occur in the clinical practice

351 Fourth, this study was performed only with one type of hammer. When using different hammer  
352 masses, impact signals could be different. Implant surface properties also has an impact on the AC  
353 implant stability (14,22,40). The effect of the AC surface properties and of the hammer mass on the  
354 variation of the implant stability and the indicator should be studied in further studies.

355 Fifth, we performed this study with a single trained operator. It is likely that the observed signals  
356 may vary with operator changes due to differences in hammer usage and striking forces. This is one  
357 of the important issues for clinical transfer that needs to be assessed in future studies.

## Conclusions

This study shows that an impact hammer can be employed in order to estimate the AC primary fixation without needing to determine the thickness of soft tissue between 10 and 30 mm of STT. The same indicator  $I$  corresponding to the impact momentum can be used indifferently. These results, together with the previous results obtained in cadavers (27) show the feasibility of the development of a medical device dedicated to the estimation of the AC implant stability, which could be used as a decision support system in a patient specific manner by orthopedic surgeons. However, clinical trials are necessary to assess the performance of the approach in the operating room.

371 **Funding:**

372 This work was supported by the French National Research Agency (ANR) through 15  
373 EMERGENCE program (project WaveImplant n°ANR-11-EMMA-039) and the PRTS program  
374 (project OsseoWave n°ANR-13-PRTS-0015-02). This work has received funding from the European  
375 Research Council (ERC) under the European Union's Horizon 2020 research and innovation  
376 program (grant agreement No 682001, project ERC Consolidator Grant 2015 BoneImplant).

377

378 **Conflicts of interest : none.**

379

380

381



382

383 **References**

- 384 1. Michel A, Bosc R, Sailhan F, Vayron R, Haiat G. Ex vivo estimation of cementless  
385 acetabular cup stability using an impact hammer. *Med Eng Phys.* 2016 Feb;38(2):80–6.
- 386 2. Perona PG, Lawrence J, Paprosky WG, Patwardhan AG, Sartori M. Acetabular  
387 micromotion as a measure of initial implant stability in primary hip arthroplasty. An in vitro  
388 comparison of different methods of initial acetabular component fixation. *J Arthroplasty.* 1992  
389 Dec;7(4):537–47.
- 390 3. Adler E, Stuchin SA, Kummer FJ. Stability of press-fit acetabular cups. *J Arthroplasty.*  
391 1992 Sep;7(3):295–301.
- 392 4. Hamilton WG, Calendine CL, Beykirch SE, Hopper RHJ, Engh CA. Acetabular fixation  
393 options: first-generation modular cup curtain calls and caveats. *J Arthroplasty.* 2007 Jun;22(4  
394 Suppl 1):75–81.
- 395 5. Kwong LM, O'Connor DO, Sedlacek RC, Krushell RJ, Maloney WJ, Harris WH. A  
396 quantitative in vitro assessment of fit and screw fixation on the stability of a cementless  
397 hemispherical acetabular component. *J Arthroplasty.* 1994 Apr;9(2):163–70.
- 398 6. Wilson MJ, Hook S, Whitehouse SL, Timperley AJ, Gie GA. Femoral impaction bone  
399 grafting in revision hip arthroplasty: 705 cases from the originating centre. *Bone Jt J.* 2016  
400 Dec;98–B(12):1611–9.
- 401 7. Mathieu V, Vayron R, Richard G, Lambert G, Naili S, Meningaud J-P, et al.  
402 Biomechanical determinants of the stability of dental implants: influence of the bone-implant  
403 interface properties. *J Biomech.* 2014 Jan 3;47(1):3–13.
- 404 8. Michel A, Nguyen V-H, Bosc R, Vayron R, Hernigou P, Naili S, et al. Finite element  
405 model of the impaction of a press-fitted acetabular cup. *Med Biol Eng Comput.* 2016 Aug 4;
- 406 9. Pierce TP, Cherian JJ, Jauregui JJ, Elmallah RDK, Mont MA. Outcomes of post-operative  
407 periprosthetic acetabular fracture around total hip arthroplasty. *Expert Rev Med Devices.* 2015  
408 May;12(3):307–15.
- 409 10. Zietz C, Fritsche A, Klues D, Mittelmeier W, Bader R. [Influence of acetabular cup  
410 design on the primary implant stability : an experimental and numerical analysis]. *Orthopade.* 2009  
411 Nov;38(11):1097–105.
- 412 11. Baleani M, Fognani R, Toni A. Initial stability of a cementless acetabular cup design:  
413 experimental investigation on the effect of adding fins to the rim of the cup. *Artif Organs.* 2001  
414 Aug;25(8):664–9.

415 12. Clarke HJ, Jinnah RH, Warden KE, Cox QG, Curtis MJ. Evaluation of acetabular stability  
416 in uncemented prostheses. *J Arthroplasty*. 1991 Dec;6(4):335–40.

417 13. Curtis MJ, Jinnah RH, Wilson VD, Hungerford DS. The initial stability of uncemented  
418 acetabular components. *J Bone Joint Surg Br*. 1992 May;74(3):372–6.

419 14. Markel D, Day J, Siskey R, Liepins I, Kurtz S, Ong K. Deformation of metal-backed  
420 acetabular components and the impact of liner thickness in a cadaveric model. *Int Orthop*. 2011  
421 Aug;35(8):1131–7.

422 15. Saleh KJ, Bear B, Bostrom M, Wright T, Sculco TP. Initial stability of press-fit acetabular  
423 components: an in vitro biomechanical study. *Am J Orthop Belle Mead NJ*. 2008 Oct;37(10):519–  
424 22.

425 16. Pastrav LC, Jaecques SVN, Mulier M, Van Der Perre G. Detection of the insertion end  
426 point of cementless hip prostheses using the comparison between successive frequency response  
427 functions. *J Appl Biomater Biomech JABB*. 2008 Apr;6(1):23–9.

428 17. Varini E, Cristofolini L, Traina F, Viceconti M, Toni A. Can the rasp be used to predict  
429 intra-operatively the primary stability that can be achieved by press-fitting the stem in cementless  
430 hip arthroplasty? *Clin Biomech Bristol Avon*. 2008 May;23(4):408–14.

431 18. Henys P, Capek L, Fencel J, Prochazka E. Evaluation of acetabular cup initial fixation by  
432 using resonance frequency principle. *Proc Inst Mech Eng [H]*. 2015 Jan;229(1):3–8.

433 19. Henys P, Capek L. Material model of pelvic bone based on modal analysis: a study on the  
434 composite bone. *Biomech Model Mechanobiol*. 2016 Aug 25;

435 20. Rowlands A, Duck FA, Cunningham JL. Bone vibration measurement using ultrasound:  
436 application to detection of hip prosthesis loosening. *Med Eng Phys*. 2008 Apr;30(3):278–84.

437 21. Smith TO, Hilton G, Toms AP, Donell ST, Hing CB. The diagnostic accuracy of  
438 acetabular labral tears using magnetic resonance imaging and magnetic resonance arthrography: a  
439 meta-analysis. *Eur Radiol*. 2011 Apr;21(4):863–74.

440 22. Sakai R, Kikuchi A, Morita T, Takahira N, Uchiyama K, Yamamoto T, et al. Hammering  
441 sound frequency analysis and prevention of intraoperative periprosthetic fractures during total hip  
442 arthroplasty. *Hip Int J Clin Exp Res Hip Pathol Ther*. 2011 Dec;21(6):718–23.

443 23. Pastrav LC, Jaecques SV, Jonkers I, Perre GV der, Mulier M. In vivo evaluation of a  
444 vibration analysis technique for the per-operative monitoring of the fixation of hip prostheses. *J*  
445 *Orthop Surg*. 2009 Apr 9;4:10.

446 24. Mathieu V, Michel A, Flouzat Lachaniette C-H, Poignard A, Hernigou P, Allain J, et al.  
447 Variation of the impact duration during the in vitro insertion of acetabular cup implants. *Med Eng*  
448 *Phys*. 2013 Nov;35(11):1558–63.

- 449 25. Michel A, Bosc R, Mathieu V, Hernigou P, Haiat G. Monitoring the press-fit insertion of  
450 an acetabular cup by impact measurements: influence of bone abrasion. *Proc Inst Mech Eng [H]*.  
451 2014 Oct;228(10):1027–34.
- 452 26. Michel A, Bosc R, Vayron R, Haiat G. In vitro evaluation of the acetabular cup primary  
453 stability by impact analysis. *J Biomech Eng*. 2015 Mar;137(3).
- 454 27. Michel A, Bosc R, Meningaud J-P, Hernigou P, Haiat G. Assessing the Acetabular Cup  
455 Implant Primary Stability by Impact Analyses: A Cadaveric Study. *PloS One*.  
456 2016;11(11):e0166778.
- 457 28. Scholl L, Schmidig G, Faizan A, TenHuisen K, Nevelos J. Evaluation of surgical  
458 impaction technique and how it affects locking strength of the head-stem taper junction. *Proc Inst*  
459 *Mech Eng [H]*. 2016 Jul 1;230(7):661–7.
- 460 29. Vayron R, Mathieu V, Michel A, Haiat G. Assessment of in vitro dental implant primary  
461 stability using an ultrasonic method. *Ultrasound Med Biol*. 2014 Dec;40(12):2885–94.
- 462 30. Meredith N, Alleyne D, Cawley P. Quantitative determination of the stability of the  
463 implant-tissue interface using resonance frequency analysis. *Clin Oral Implants Res*. 1996  
464 Sep;7(3):261–7.
- 465 31. Vayron R, Soffer E, Anagnostou F, Haiat G. Ultrasonic evaluation of dental implant  
466 osseointegration. *J Biomech*. 2014 Nov 7;47(14):3562–8.
- 467 32. Lannocca M, Varini E, Cappello A, Cristofolini L, Bialoblocka E. Intra-operative  
468 evaluation of cementless hip implant stability: a prototype device based on vibration analysis. *Med*  
469 *Eng Phys*. 2007 Oct;29(8):886–94.
- 470 33. Le Cann S, Galland A, Rosa B, Le Corroller T, Pithieux M, Argenson J-N, et al. Does  
471 surface roughness influence the primary stability of acetabular cups? A numerical and  
472 experimental biomechanical evaluation. *Med Eng Phys*. 2014 Sep;36(9):1185–90.
- 473 34. Spears IR, Morlock MM, Pfleiderer M, Schneider E, Hille E. The influence of friction and  
474 interference on the seating of a hemispherical press-fit cup: a finite element investigation. *J*  
475 *Biomech*. 1999 Nov;32(11):1183–9.
- 476 35. Spears IR, Pfleiderer M, Schneider E, Hille E, Morlock MM. The effect of interfacial  
477 parameters on cup-bone relative micromotions. A finite element investigation. *J Biomech*. 2001  
478 Jan;34(1):113–20.
- 479 36. Won CH, Hearn TC, Tile M. Micromotion of cementless hemispherical acetabular  
480 components. Does press-fit need adjunctive screw fixation? *J Bone Joint Surg Br*. 1995  
481 May;77(3):484–9.

37. MacKenzie JR, Callaghan JJ, Pedersen DR, Brown TD. Areas of contact and extent of gaps with implantation of oversized acetabular components in total hip arthroplasty. Clin Orthop. 1994 Jan;(298):127–36.
38. Michel A, Bosc R, Chappard C, Takano N, Haiat G. Biomechanical behavior of the acetabular cup implant a finite element study. Computer Methods in Biomechanics and Biomedical Engineering. submitted;
39. Poumarat G, Squire P. Comparison of mechanical properties of human, bovine bone and a new processed bone xenograft. Biomaterials. 1993 Apr;14(5):337–40.
40. Small SR, Berend ME, Howard LA, Rogge RD, Buckley CA, Ritter MA. High initial stability in porous titanium acetabular cups: a biomechanical study. J Arthroplasty. 2013 Mar;28(3):510–6.

498 Legends

499

500 Figure 1: Schematic representation of the experimental set-up.

501

502 Figure 2: Experimental protocol employed in the present study.

503

504 Figure 3: Averaged variations of the force as a function of time corresponding to the 25 impacts  
505 realized during the impaction procedure for 6 different conditions of implant insertions. The black  
506 (respectively grey) signals correspond to 10 mm (respectively 30 mm) of soft tissue thickness  
507 (STT). The solid (respectively dotted and dashed) lines correspond to the implant stability equal to  
508 31 N (respectively 63.4 N and 72.80 N). The two vertical lines indicate the time window  
509 considered to compute the value of the indicator  $I_m$ .

510



511 Figure 4: Variation of the tangential stability  $F$  as a function of the averaged value of the indicator  
512  $I_m$  for all data pooled from all bone samples and configurations. The circles (respectively the stars)  
513 show the data corresponding to a value equal to 10 mm (respectively 30 mm) for the soft tissue  
514 thickness. The black (respectively grey) line corresponds to the linear regression analysis obtained  
515 for a value equal to 10 mm (respectively 30 mm) for the soft tissue thickness.

516


517 Figure 5: Representation of the average and of the standard deviation of the indicator  $I$  (black  
518 segments) and of the pull-out force (grey segments) as a function of the soft tissue thickness (for  
519 the indicator) and of the implant and cavity diameter

520

521

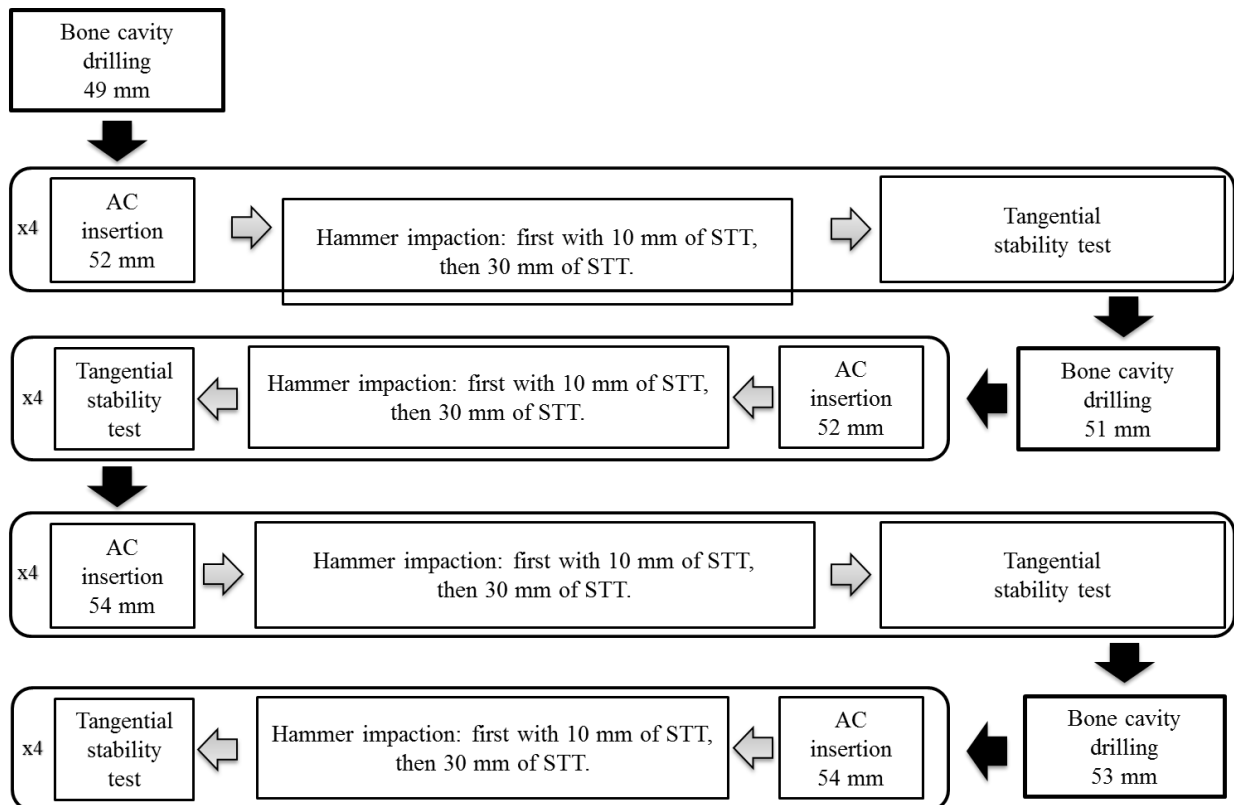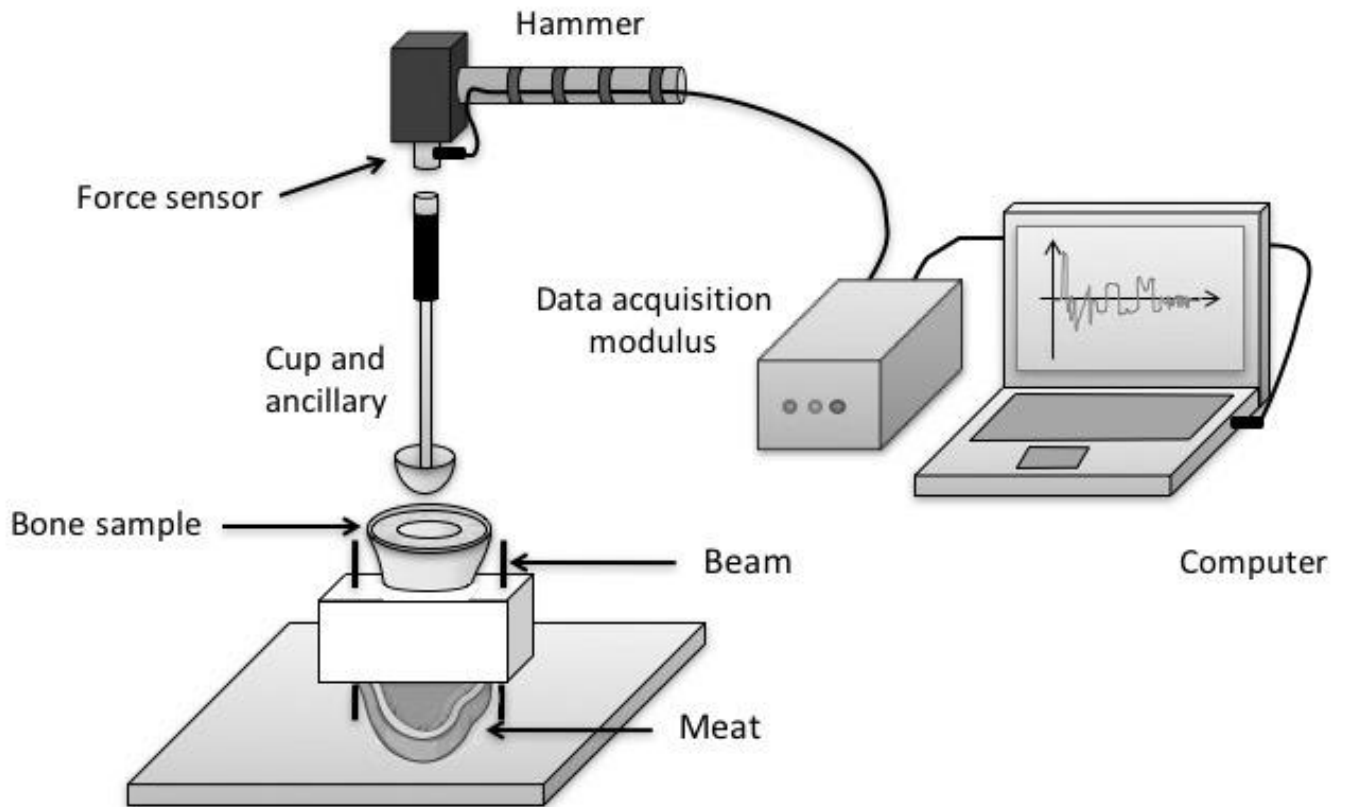


527

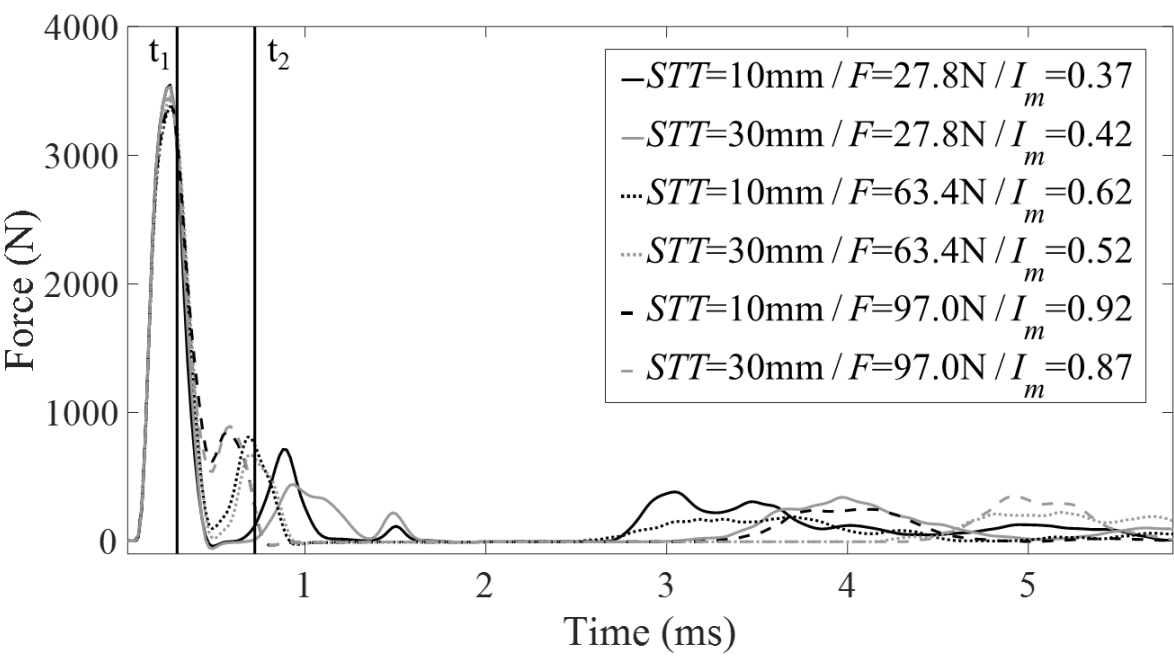

528

529

530

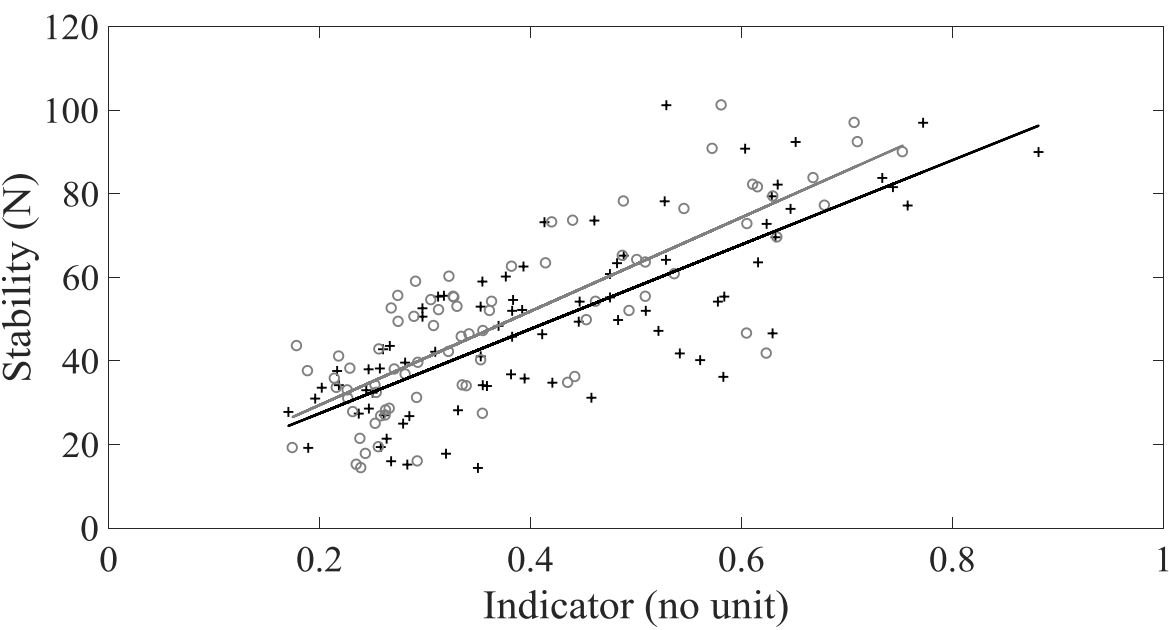

531

532

533

